

C4i *communication*

EXPERIENCE THE DIFFERENCE
YOUR SECURITY & SAFETY PRODUCTS

MEDICAL CAP SERIES



LEARN MORE:

<http://c4communication.com>

MEDICAL CAP C4MC

Class I medical supplies

Used for general isolation in outpatient, ward and laboratory of medical institution.

It is made of SS non-woven fabric by cutting and sewing.

Average size

Product name : Medical cap

Packing specification : 20/ bag 60 bags/box 1200 pieces/box

Intended use : used for general isolation in outpatient, ward, laboratory, etc.

Main structure : non-woven fabric as the main material, through tailoring and sewing.

Notes :

(1) please read the instructions carefully before use and use within the warranty period.

(2) after use, the product shall be disposed according to the requirements of the hospital or the environmental protection department.

Instructions for use :

(1) before using the product, attention should be paid to the packaging, production batch number and expiry date.

(2) non-sterile, disposable.

(3) open the package when using and carry out routine operation as required.

(4) routine treatment is required after use.

Storage method : well ventilated, stored at room temperature.



Scope of application

Used for general isolation in out-patient, ward and laboratory of medical institution.



The characteristics of

SS non-woven fabric, strong and durable, one-way breathable, exhaust internal heat, blocking external gas,




Model and specification

Specifications

Outer diameter : 320mm±10mm

The inner diameter : 160mm±10mm

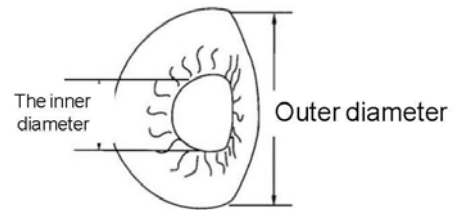


Storage

Medical caps should be stored in a warehouse with relative humidity not exceeding 80%, no corrosive gas, cool, dry and good ventilation.

The outer packing

Isolation cap packing standard

Specification:	general purpose
Number of packages:	1200 sets/carton
Gross weight:	9.65kg/carton
Net weight:	7.95 kg/carton
Size:	60*40*40cm
Unit:	0.096 cubic meters

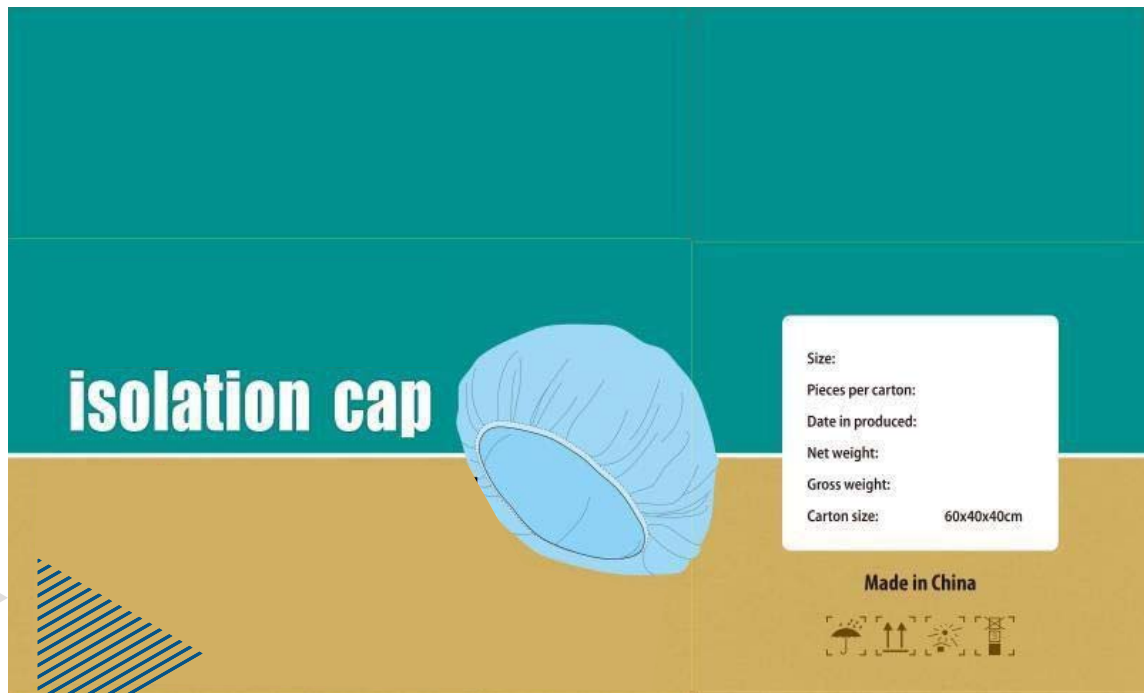

Relevant qualifications

FDA Registration Certificate
FDA 注册证明
Fiscal Year 2020


COMPANY	[REDACTED]
ADDRESS	[REDACTED]

Owner / Operator Number:	[REDACTED]
Device Listing #:	See Annex
Expiration Date:	Dec. 31, 2020

Proprietary Name	Product Codes	Device Class	Listing Number	Establishment Operations
Non-surgical isolation gown	OEA	1	[REDACTED]	Manufacturer
COVER, SHOE, OPERATINGROOM	FXP	1	[REDACTED]	Manufacturer
Face mask (except N95 respirator) for general public/healthcare personnel per IIE guidance	OKR	1	[REDACTED]	Manufacturer
CAP, SURGICAL	FYF	1	[REDACTED]	Manufacturer

[REDACTED]

Apr. 09, 2020
(Date)



Quality Management

Declaration of Conformity

HUACETONG

Certificate No.: WJ [REDACTED]

Applicant: [REDACTED]

Address: [REDACTED]

Manufacturer: [REDACTED]

Address: [REDACTED]

Product Name: protective cap

Model No.: All code

Trade Mark: /

Test Standard: EN 14126:2003

Test Report Number(s): WJ [REDACTED]

PPE directive (EU) 2016/425

The CE markings as shown below can be affixed on the product after preparation of necessary conformity documentation, as stipulated in article 10 of the Council Directive 93/68/EEC.

CE

Tony Bi
 Tony Bi
 Technical Director

Mar. 24, 2020

Shenzhen Huacetong Testing and Certification Co., Ltd.
 Building B, Xixiaochang, No.233, Xixiang Street, Bao'an District, Shenzhen, China.
 Web: www.szctifab.com Tel: 86-755-23925224 E-mail: cti_lab@foxmail.com



LEARN MORE: c4icommunication.com

FOR MORE INFORMATION: contact@c4icommunication.com or +1 (302) 981 1340